

FIG. 1

Pipetter Device 200

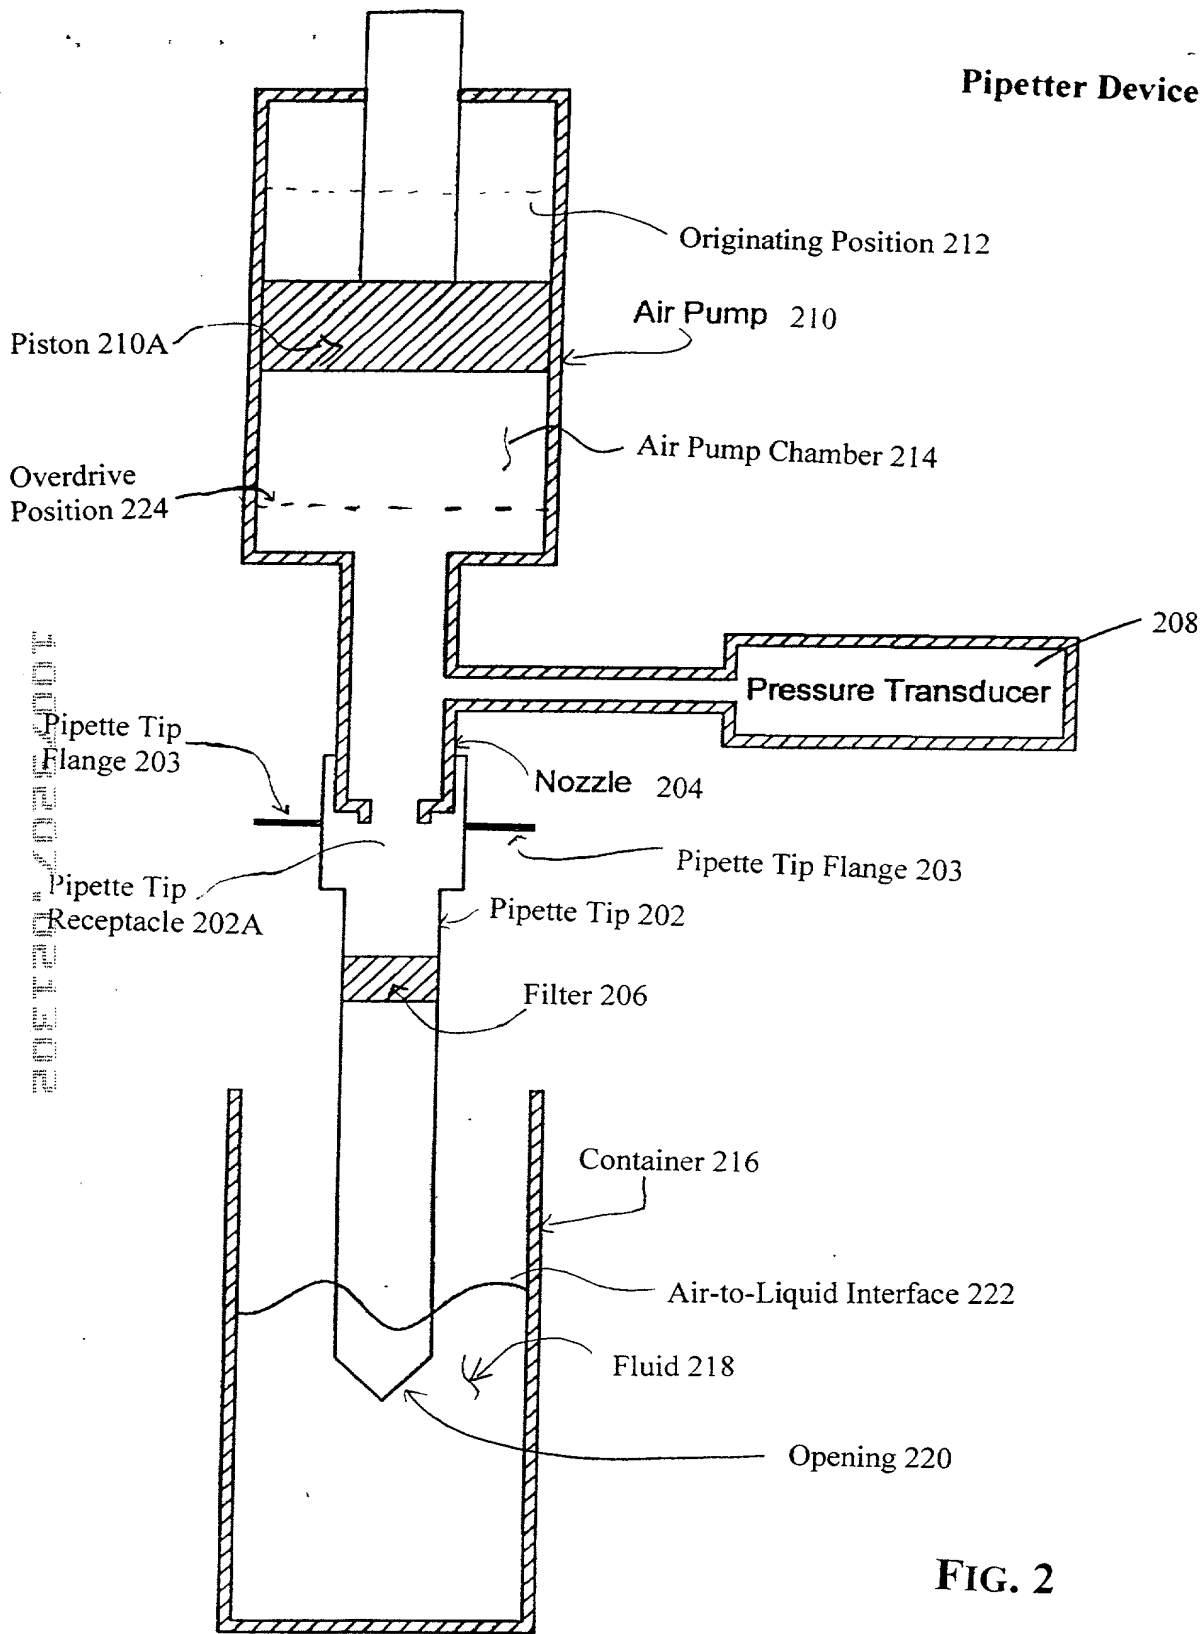


FIG. 2

20250720 2025/07/20

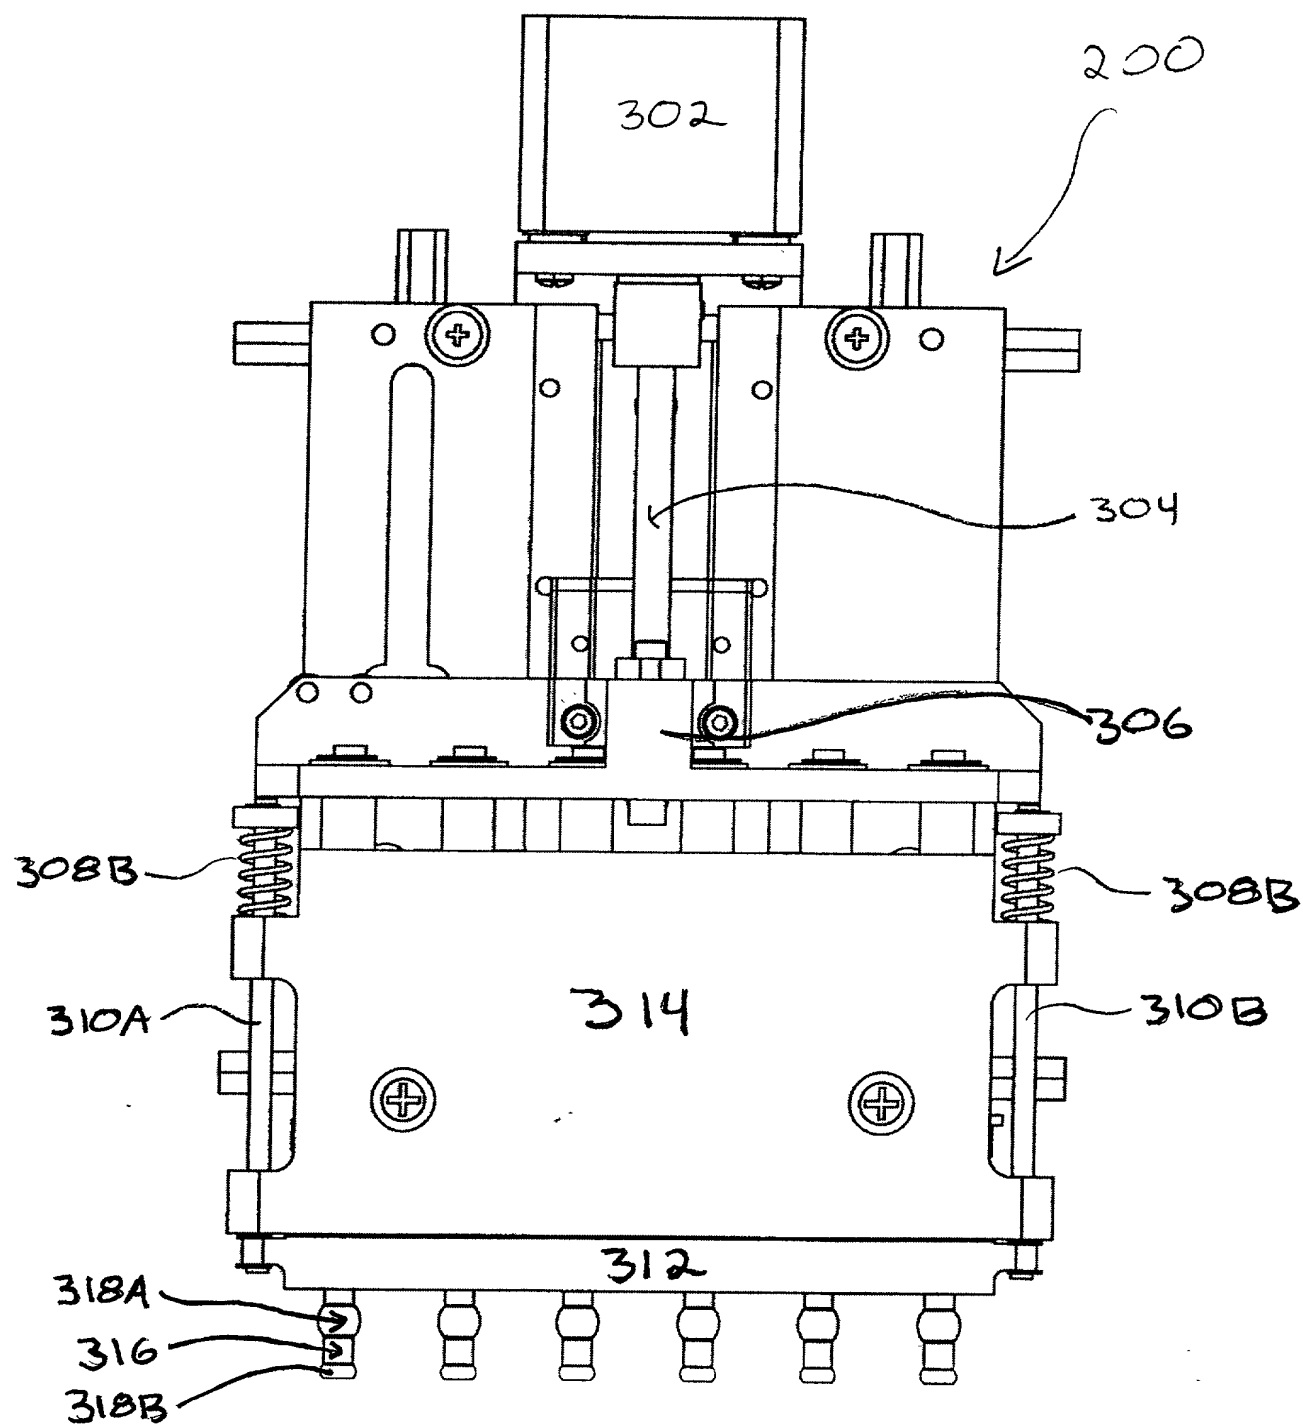


FIG. 3

2025-2026-2027

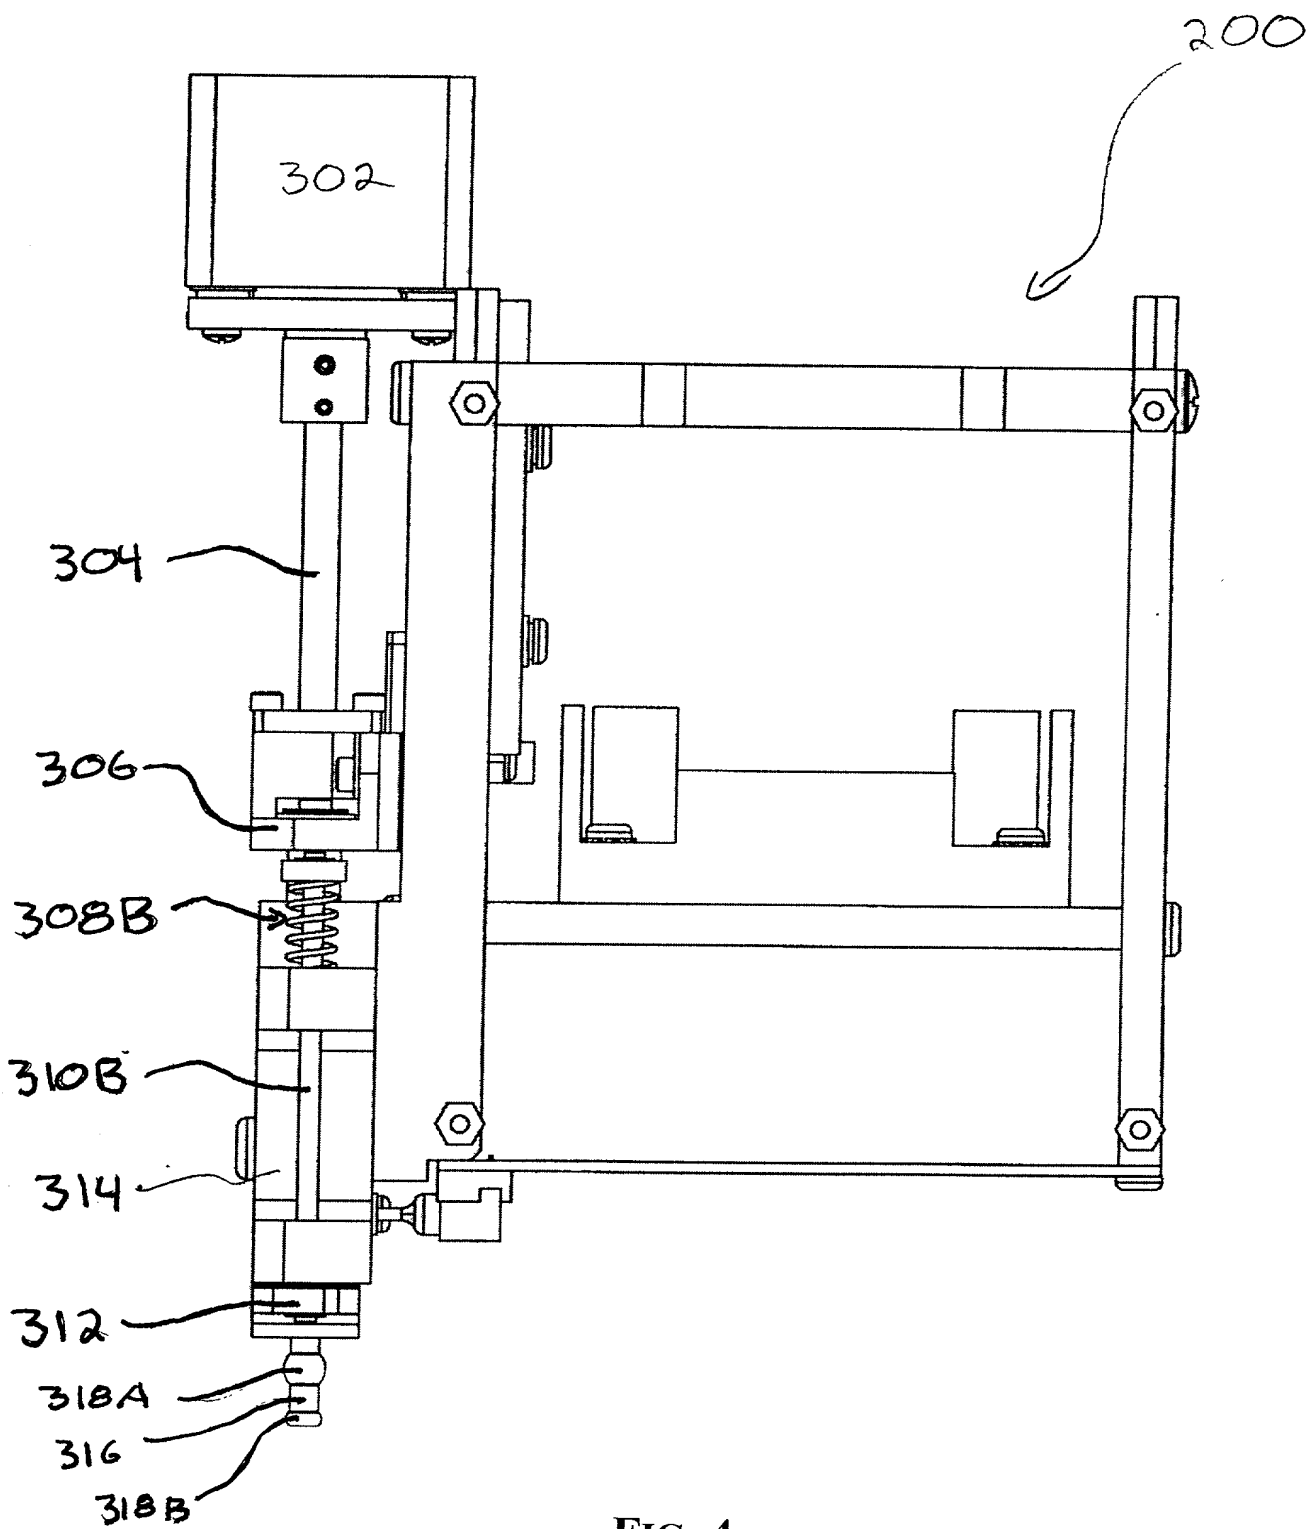


FIG. 4

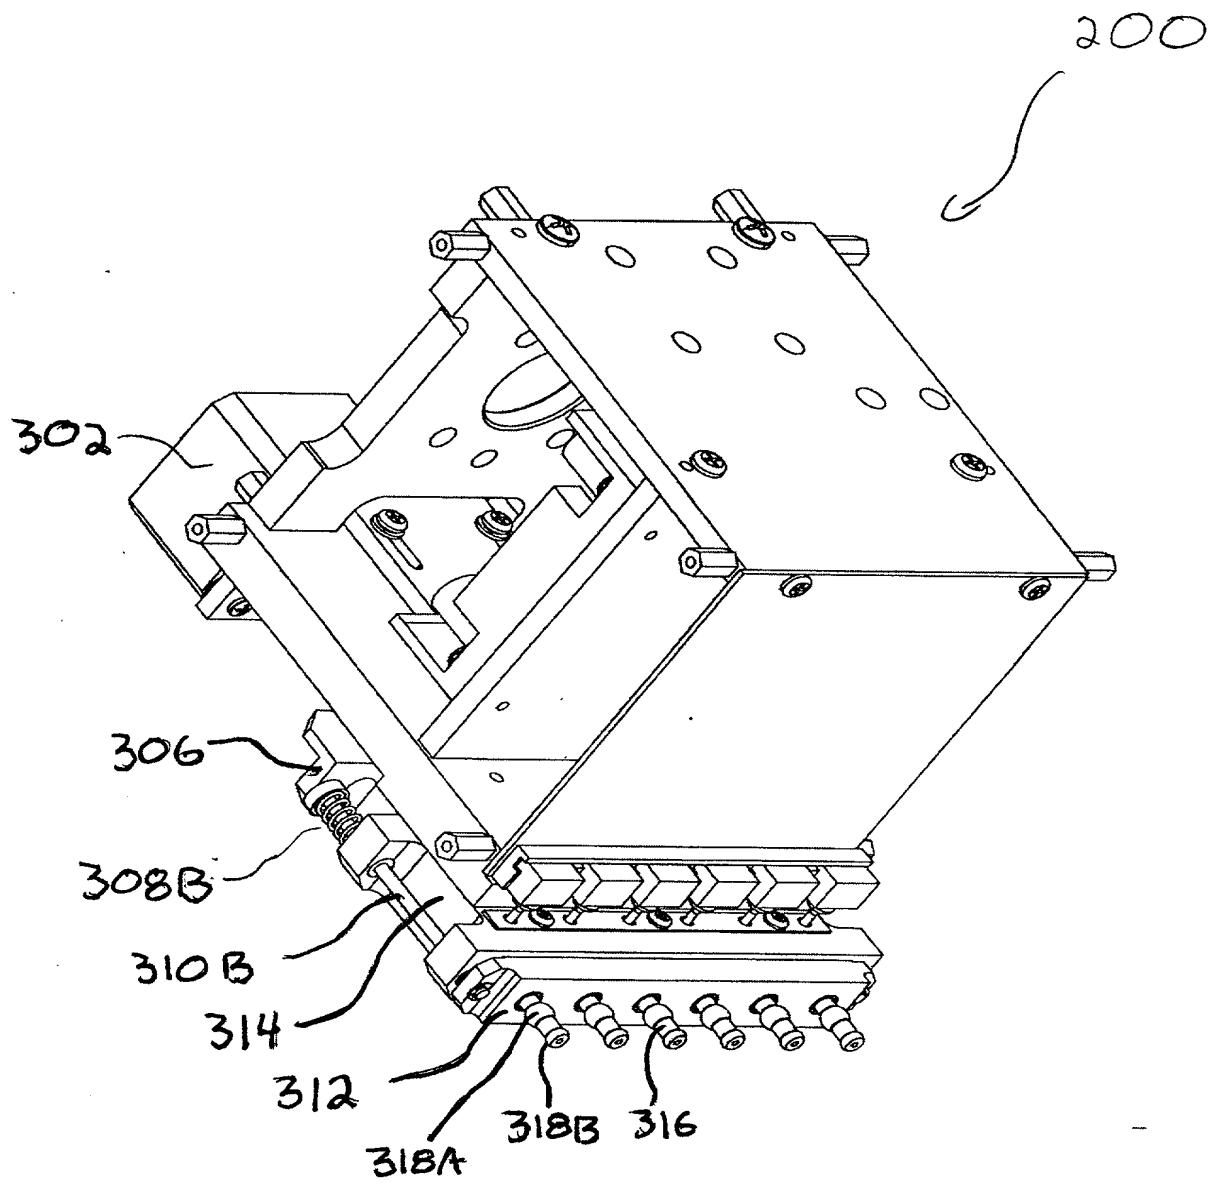


FIG. 5

2025-12-20 14:02:00

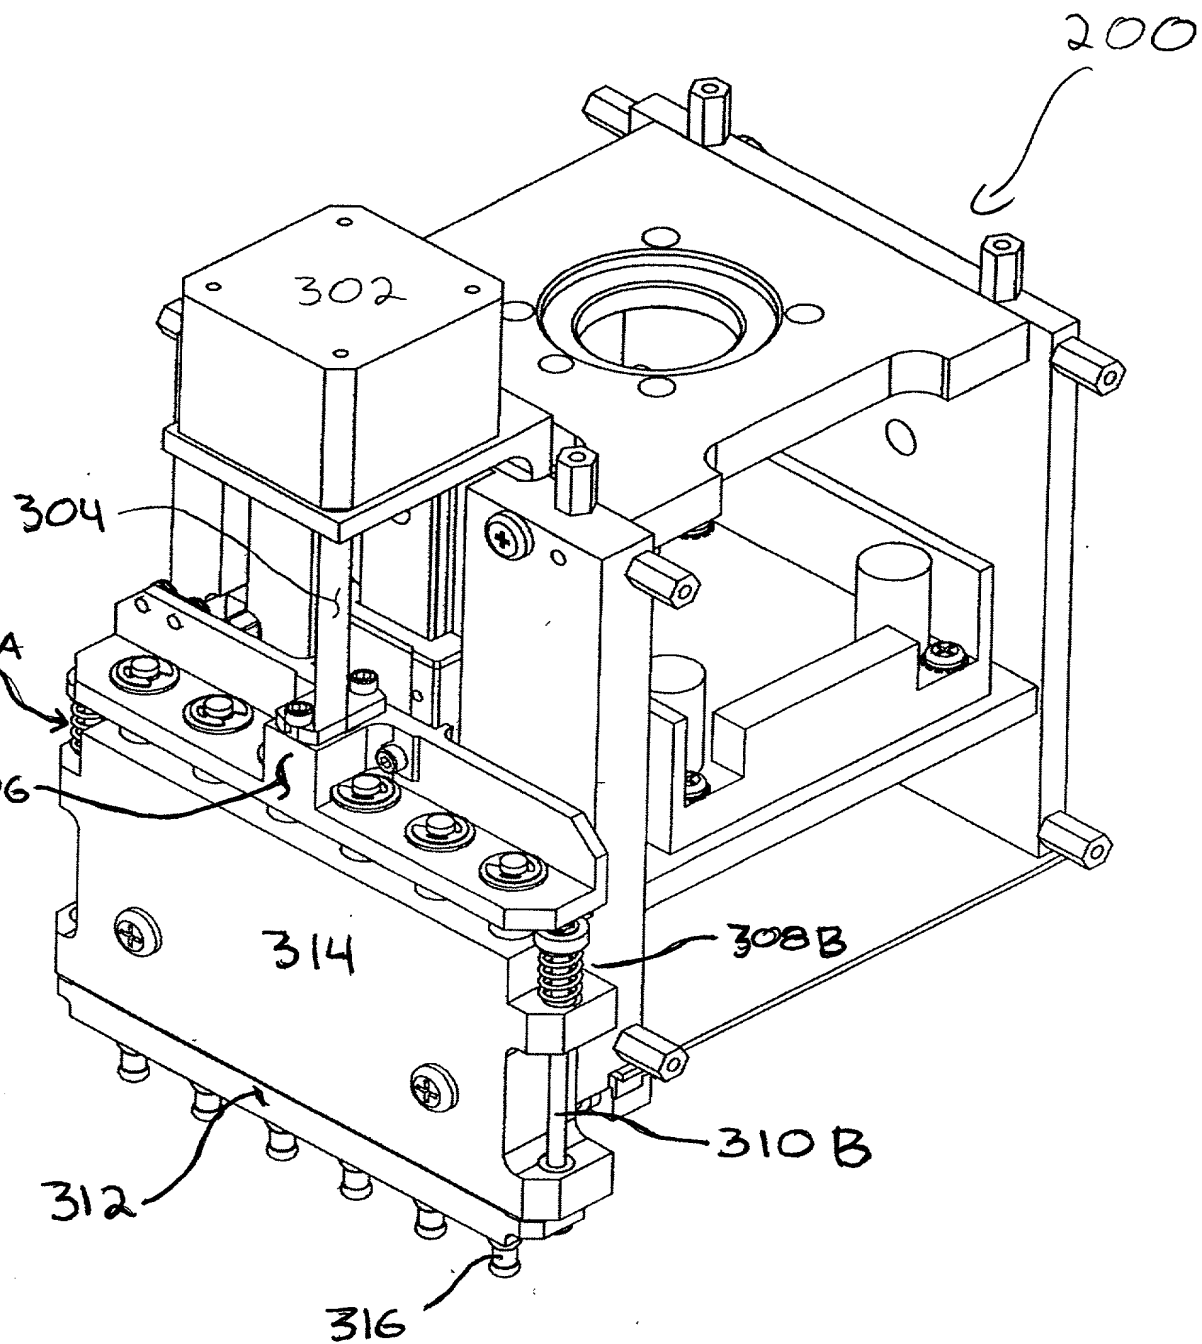


FIG. 6

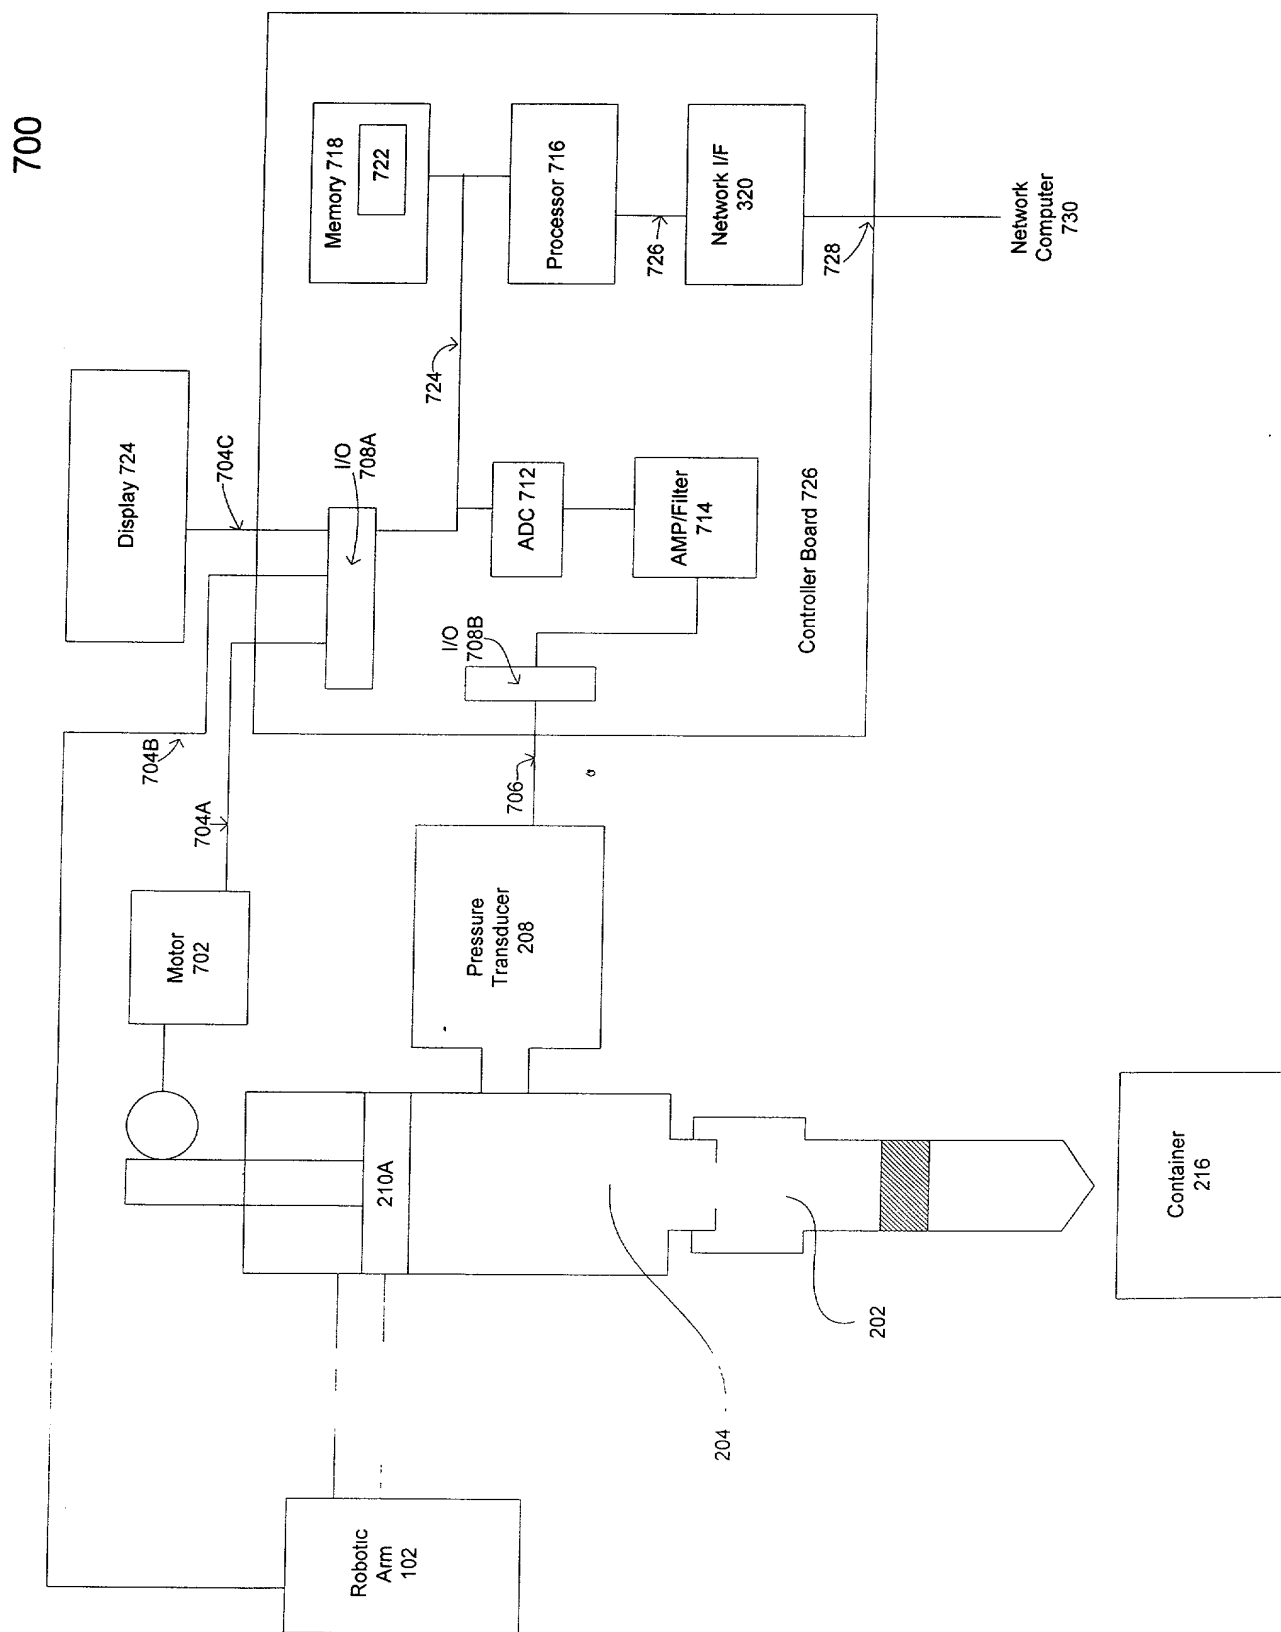


FIG. 7

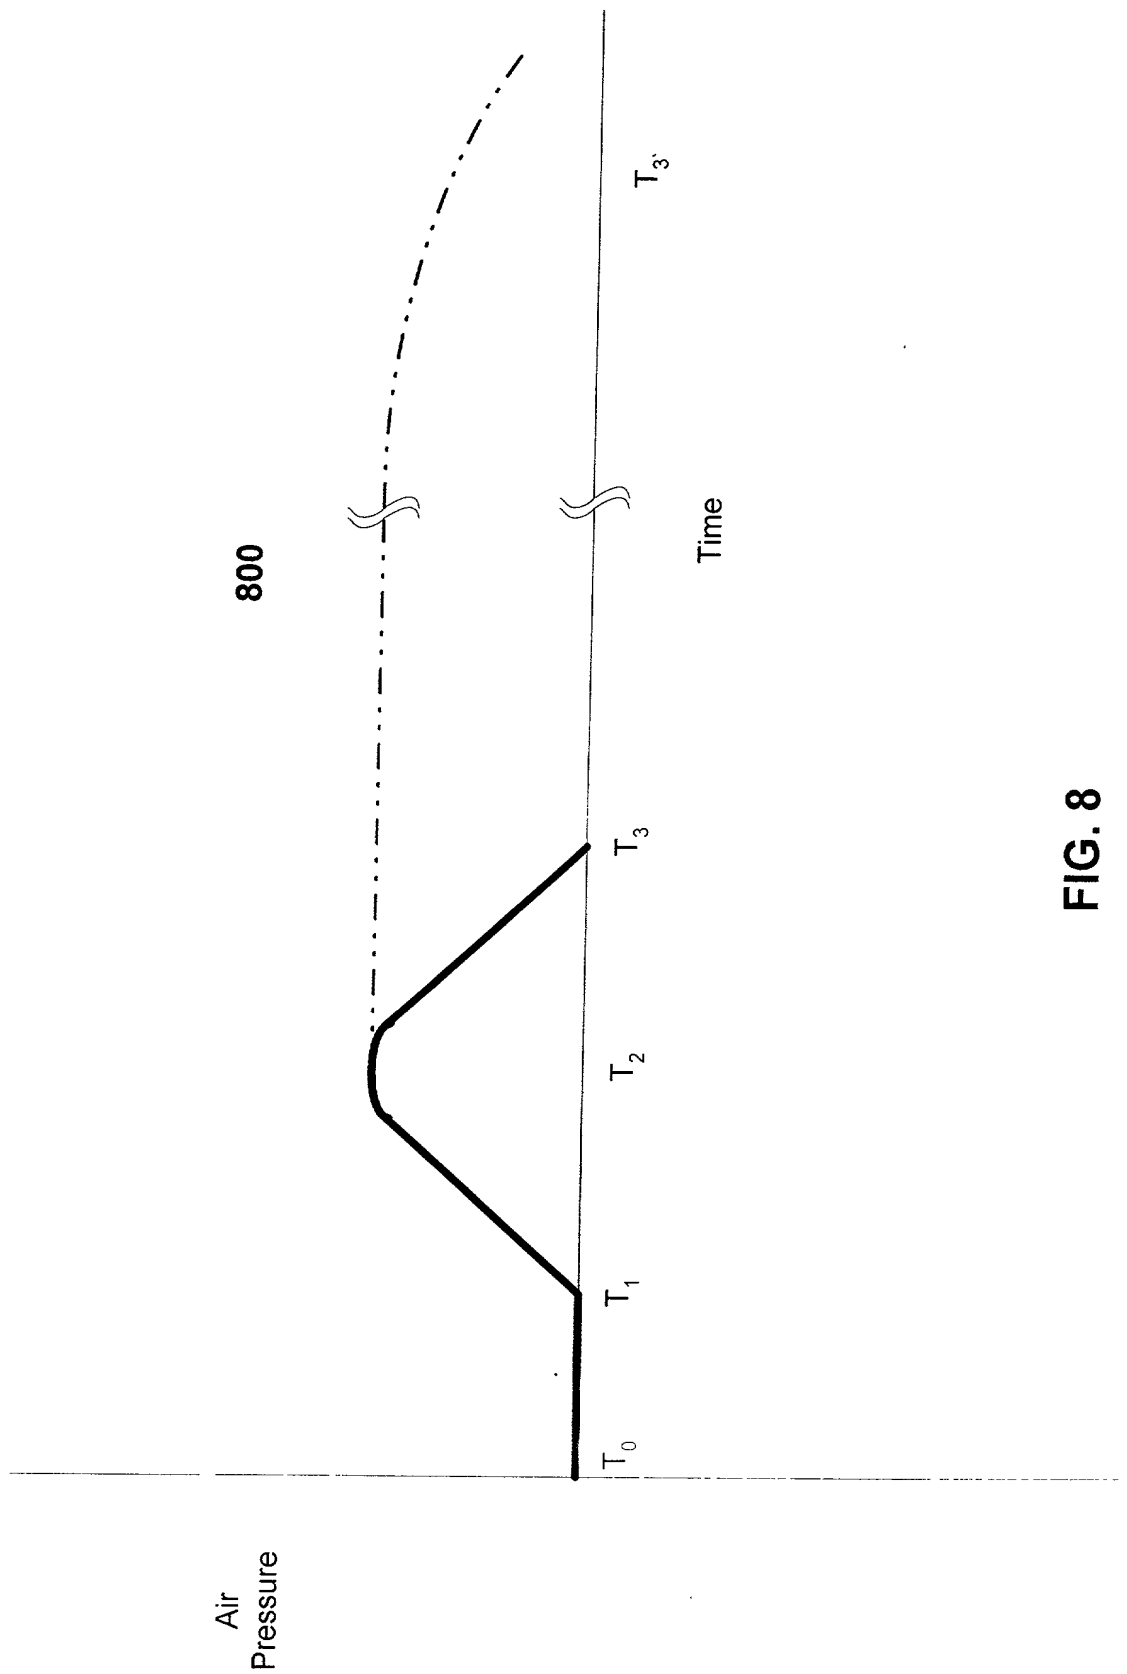


FIG. 8

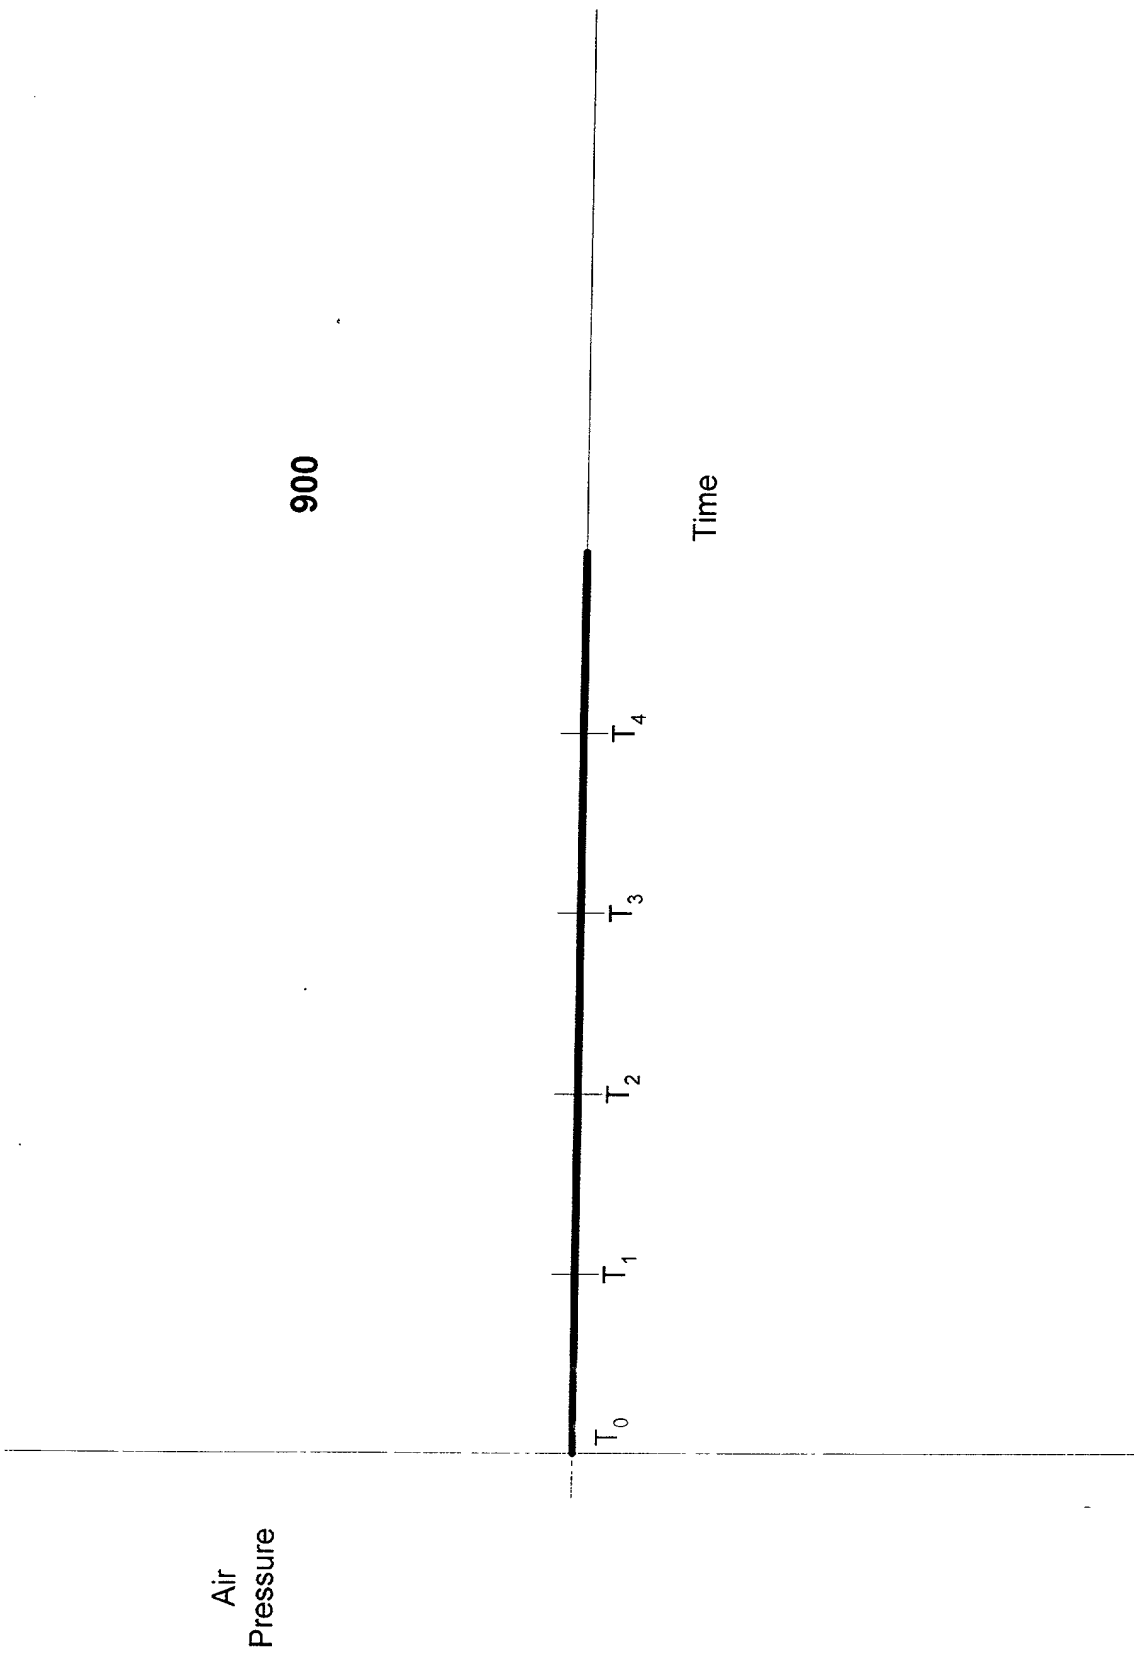


FIG. 9


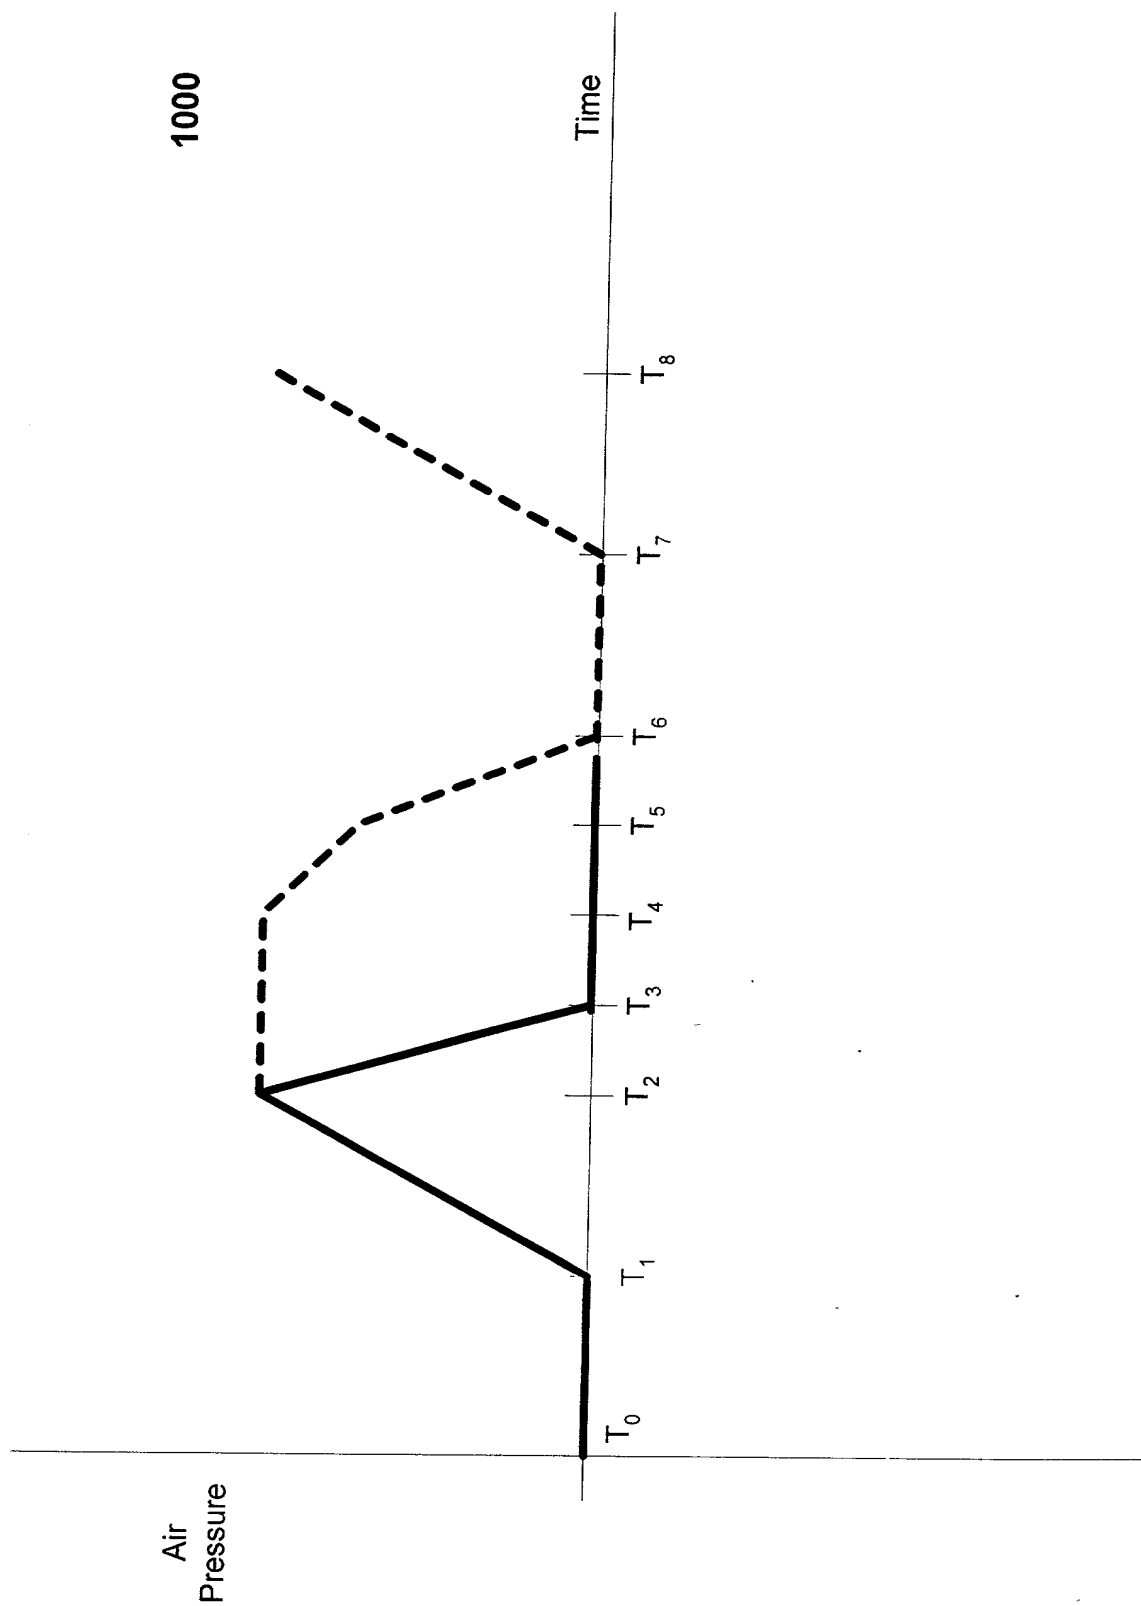


FIG. 10

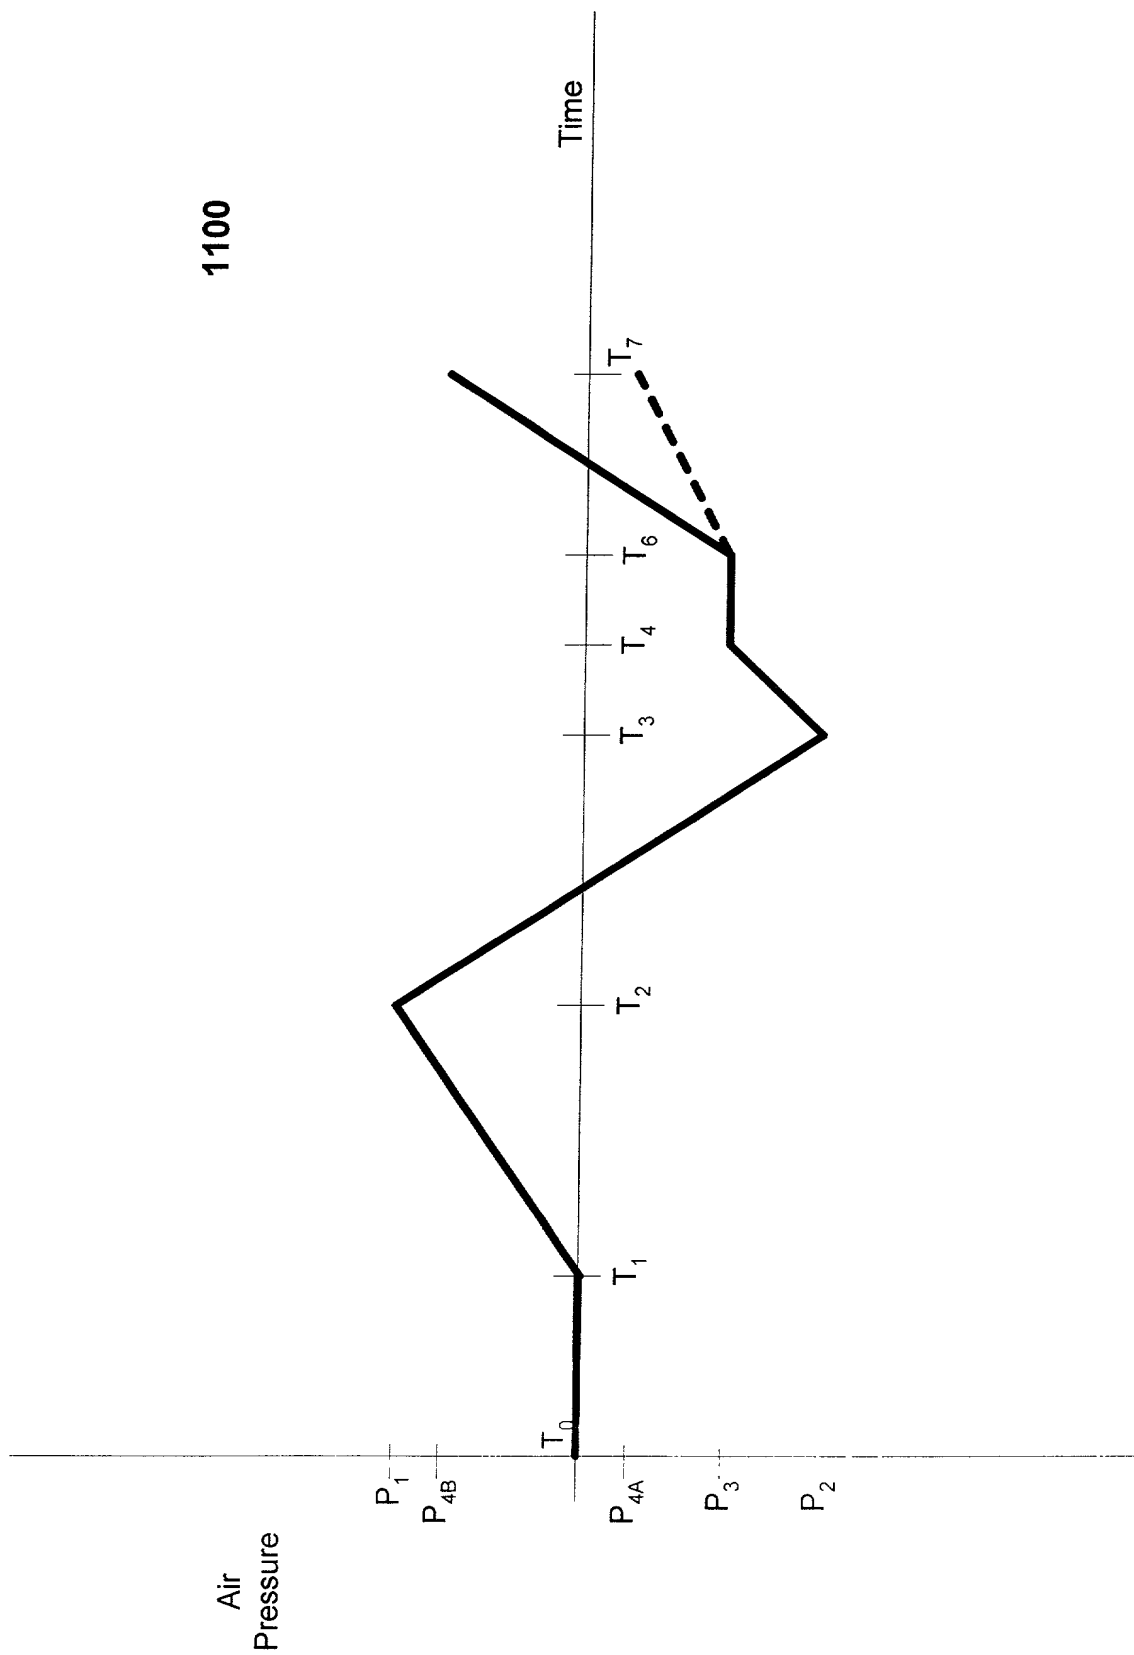

1100

FIG. 11

1200

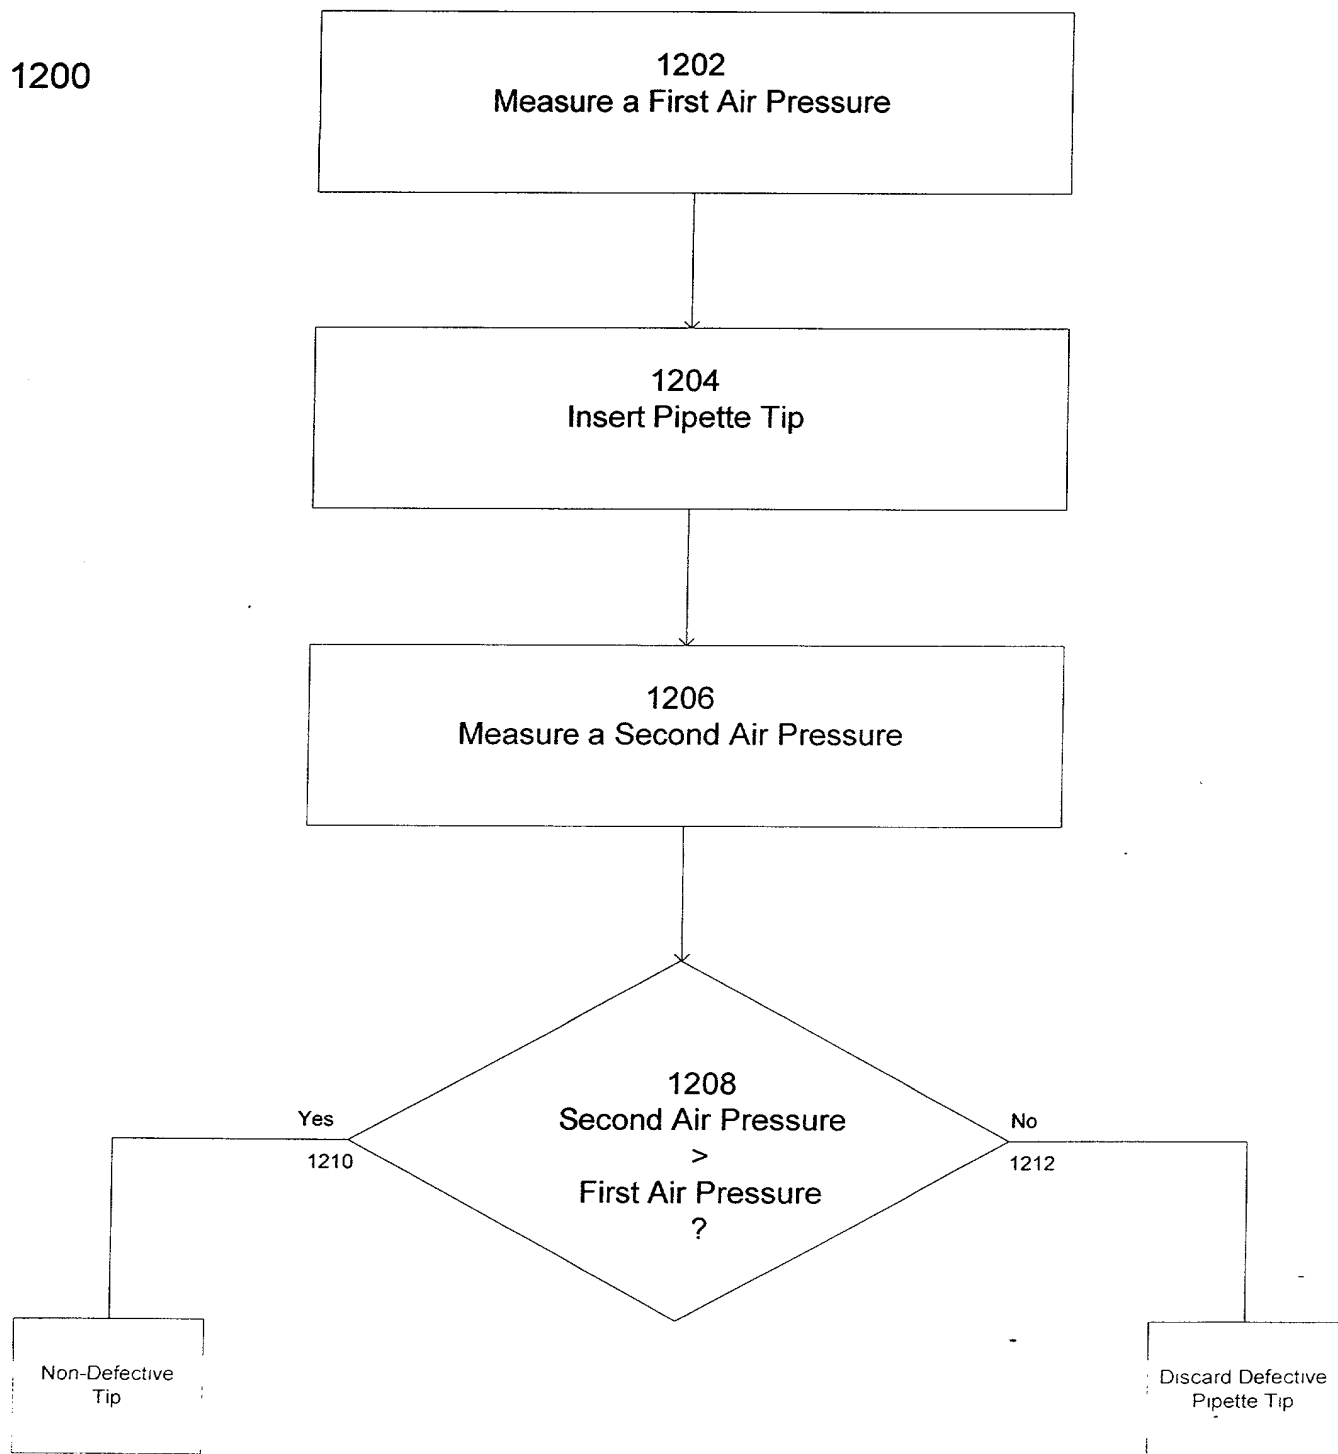


FIG. 12

2025-07-20 10:00:00

1300

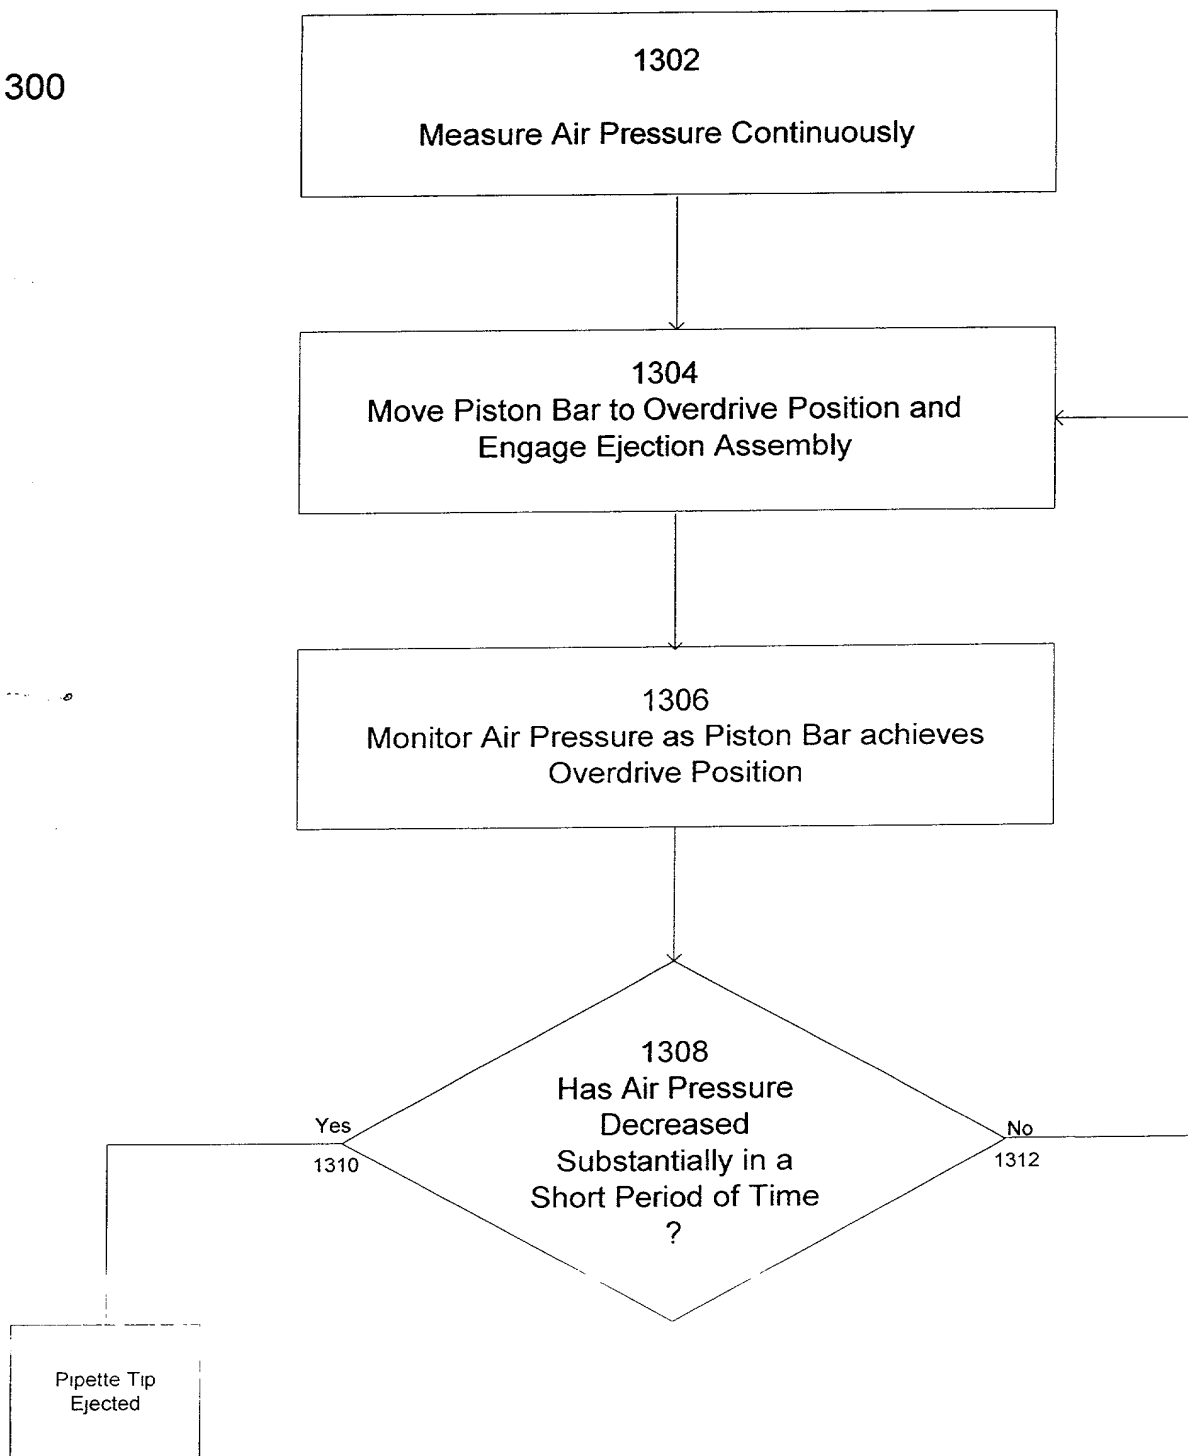


FIG. 13